PRODONT HOLLIGER I A company of ACTEON GROUP
3, La Marnasse I 63880 OLLIERGUES I France

CE

Ce Matériel est destiné à un usage professionnel, il doit être nettoyé, désinfecté et stérilisé avant chaque utilisation. Le nettoyage et la désinfection sont à réaliser en utilisant des solutions à pH neutre en suivant scrupuleusement les indications des fournisseurs (temps de trempage et dilution). La stérilisation par autoclave est réalisable à 132°C-4 minutes ou 134°C -18 minutes. Ne pas dépasser 180°C. Durant le cycle de nettoyage ne pas traiter ces instruments avec des articles en acier inoxydable. Eviter que les instruments ne s'entrechoquent.

This Equipment is intended for professional use, it must be cleaned, disinfected and sterilized before each use. Cleaning and disinfection must be carried out using neutral pH solutions, following scrupulously the suppliers' indications (soaking time and dilution). Sterilization by autoclave is possible at 132°C/ 270°C - 4 minutes or 134°C/ 273°F -18 minutes. Do not exceed 180°C / 360°F. During the cleaning cycle do not treat these instruments with stainless steel articles. Avoid the instruments clashing.

21-10-Verso cartonnette V2.indd 1 04/10/2021 09:25:02

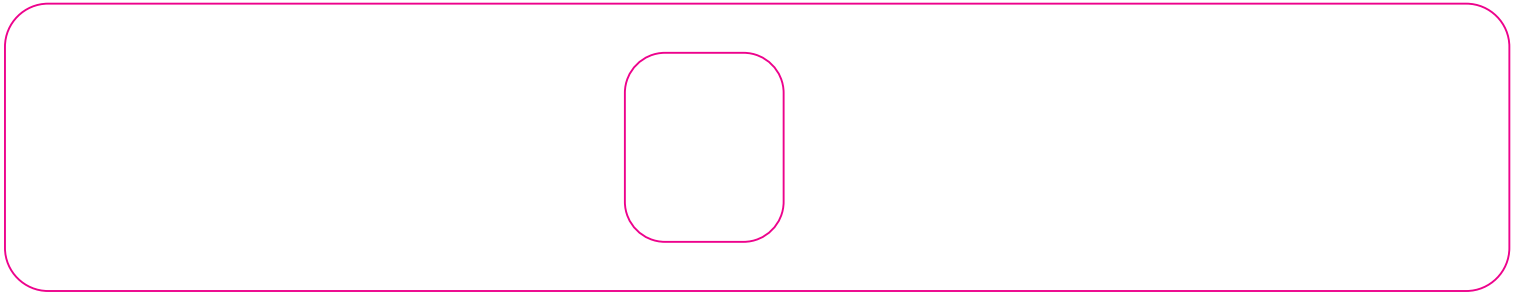

21-10-Verso cartonnette V2.indd 2 04/10/2021 09:25:02